

Manuscript received December 10, 2020; Revised December 15, 2021; accepted January 10, 2022; date of publication February 20, 2022

Digital Object Identifier (DOI): <https://doi.org/10.35882/ijeemi.v4i1.1>

This work is an open-access article and licensed under a Creative Commons Attribution-ShareAlike 4.0 International License ([CC BY-SA 4.0](https://creativecommons.org/licenses/by-sa/4.0/))



Vital Signs Monitoring Device with BPM and SpO2 Notification to the Internet of Things Based on Telegram App

Sari Luthfiyah¹, Elga Rahmah Ramadhani¹, Tri Bowo Indrato¹, and Anan Wongjan²

¹ Departement Of Electromedical Engineering Poltekkes Kemenkes Surabaya, Indonesia

² Faculty of Engineering, King Mongkut's Institute of Technology, Ladkrabang, Bangkok, 10520 Thailand

Corresponding author: Sari Luthfiyah (sarilut@poltekkesdepkes-sby.ac.id).

ABSTRACT Vital signs are an important component of monitoring the adult or child patient's progress during hospitalization, as they allow for the prompt detection of delayed recovery or adverse events. Vital signs are measured to obtain basic indicators of a patient's health status. The most common intervention performed in hospital medicine is a measurement of vital signs and these traditionally consist of blood pressure, temperature, pulse rate, and respiratory rate. Advanced monitoring systems incorporate a balanced combination of clinical and technological aspects to give an innovative healthcare outcome. Remote patient monitoring systems are rapidly becoming the core of healthcare deliveries. The paradigm shifted from traditional and manual recording to computer-based electronic records and further to smartphones as versatile and innovative healthcare monitoring systems. The purpose of this research is to design a Vital Sign Monitoring device for BPM and SpO2 Parameters with Notifications through the IoT-Based Telegram application. This device can monitor vital signs, especially BPM and SPO2 wherever the patient is and whenever, so that doctors or health workers, as well as patients, can find out their health condition. This display can be viewed via web tinger.io, then forwarded to telegram if an abnormal patient condition is found and there is an indicator light that will light up differently for each condition. This study uses the MAX30100 which is a digital sensor to detect oxygen saturation and heart rate. The results of this study have succeeded in displaying data on the IoT web and sending notifications to the Telegram application. And also, the resulting data has an error that does not exceed the allowable limit according to each parameter. The difference between heart rate readings and oxygen saturation values on the device and patient monitor is 0.015% for heart rate and 0.01% for oxygen saturation. The results of this study indicate that it is time to monitor vital signs that can be seen remotely and have a system that is an inexpensive and easy-to-operate device for health workers without interfering with activities of daily living.

INDEX TERMS Vital Sign Monitor, MAX30100, BPM, SpO2, IoT

I. Introduction

Vital signs are an important component of monitoring the adult or child patient's progress during hospitalization, as they allow for the prompt detection of delayed recovery or adverse events. Vital signs are measured to obtain basic indicators of a patient's health status. The most common intervention performed in hospital medicine is a measurement of vital signs and these traditionally consist of blood pressure, temperature, pulse rate, and respiratory rate. Continuous monitoring of vital signs by using wearable wireless devices may allow for timely detection of clinical deterioration in patients in general wards in comparison to detection by standard intermittent vital signs measurements. The heart is one of the important organs in the body that has a heavy duty and works very hard. The heart works as a pump of blood throughout the body. Everything that is consumed and also the activities that are done every day can affect the condition of the heart[1]. The heart works continuously without stopping and will decrease with increasing human age. The normal human heart rate

ranges from 60-100 beats per minute (beats per minute/bpm)[2]. A monitoring device is a device that serves to monitor a person's health condition. Monitoring is very necessary if there are symptoms of a disease that must be taken quickly so that the patient's condition does not worsen. The patient's condition can deteriorate anywhere and at any time. For that, we need a device equipped with a system that can notify doctors so that they can take action if the patient shows results less or more than normal [3]. The purpose of this study was to design a Vital Sign Monitoring Device with IoT-Based Notification Parameters (BPM and SpO2). This device can monitor vital signs, especially BPM and SPO2 wherever the patient is and whenever, so that doctors or health workers, as well as patients, can find out their health condition. This display can be viewed via web tinger.io, then forwarded to telegram if an abnormal patient condition is found and there is an indicator light that will light up differently for each condition. This study uses the MAX30100 which is a digital sensor to detect oxygen saturation and heart rate.

In a previous study, Anggi Zafia made a prototype of an Inpatient Vital Monitoring Device using a Wireless Sensor as a Physical Distancing Effort for handling Covid 19 using Zigbee [4]. A similar study was also conducted by Fahmi Farisandi and Ahmad Fatkudin on Portable Patient Diagnostics equipped with Normal/Abnormal Indicators [5]. The device was able to analyze the rate of change of BPM, and changes in the patient's body temperature. Several researchers and manufacturing companies in the medical field were conducting research and development of this system which was used for daily heart activity monitoring needs, as was done by [6] using the Max30100 sensor and Arduino microcontroller with a personal computer display with an accuracy of 92.36%. However, this system will only output BPM (Beat Per Minute) data. The other research [7] was a heart rate monitor based on a laptop interface microcontroller, using an AD8232 sensor and an Arduino Nano microcontroller, displaying ECG waveforms, bpm counts, and images of normal heart rates. Some of these studies were using laptop displays, this is inflexible for some users.

Therefore, we need a device design that can be used easily in monitoring heart rate using a PC or smartphone display at a low cost. The recording results can be known directly which is then also stored in a WEB application that is sent via internet media which is known as IoT-based. The use of IoT systems in the medical world can also facilitate the information system of a hospital [8]. Anan Wongjan, Amphawan Julsereewong, and Prasit Julsereewong made a device to measure heart rate and oxygen saturation in real-time using two LEDs, namely a red LED and an infrared LED, as well as a photodiode. The photodiode used is TCS-230 which is used to detect the intensity of light on the two LEDs reflected by the finger veins. To be able to produce readings of heart rate and oxygen saturation, this device is used on the finger. The measurement signal is processed using LabVIEW which then displays real-time heart rate per minute (BPM) and oxygen saturation readings. This device is also equipped with a probe-off alarm and a warning message when the finger is not attached to the sensor [9]. In this study, the device had a fairly large shape, besides that sensor readings are sent to a computer via NI_USB-6009 which is a data acquisition module, so it was not easy to carry anywhere and wireless communication with Bluetooth is not yet supported. In a 2019 study, Heart Rate Monitoring and Oxygen Saturation Through Smartphones was created by Arys Sulisty Utomo, et al from the Electrical Engineering Academy, made to monitor heart rate and oxygen saturation that can be monitored via a smartphone [10]. The drawback of this study was the readings of the heart rate and oxygen saturation values are different between the display on the LCD and the smartphone due to the unequal time of sending the reading data. In the same year, research was conducted on a Hypoxic Symptom Detection System Based on Oxygen Saturation and Heart Using the Arduino-Based

Fuzzy Method by Dian Bagas Setyo Budi, et al from Brawijaya University [11]. In 2013, Yessy Mega Jayanti made a Portable BPM With a Finger Sensor Based on the ATtiny2313 Microcontroller[12], there were shortcomings in this study because this device did not have a remote monitor, and RTC to find outpatient data every hour. Then it was developed by Riszqy Cahyaning Maulina who made a Heart Rate Monitoring device with a Graphic LCD equipped with an SD Card and RTC storage[13], but the drawback of this device was that its physical condition was still large and did not display BPM but instead displays a graph. Fachrul Rozie from Electrical Engineering, Tanjungpura University in 2016, developed previous research with his research, namely the design of an android-based heart rate monitoring device [14]. However, the drawback of this device is that it only has one parameter. Guruh Hariyanto, Universitas Airlangga, continued his research, Designing a digital oximeter based on the Atmega16 microcontroller and found a drawback that the device only uses one parameter and is not portable[15]. In 2017, Lokeswara Darmalaksana with his research was a portable BPM with a finger sensor equipped with RTC and SD card storage[16], but this device has the disadvantage of a device that only detects bpm and is displayed on seven segments. In 2019, the SpO2 and BPM Smartwatch Design with Android Display by Eryanda Bima Mahendra[17] were made, this research was built based on the ATmega328P microcontroller, Max30100 sensor, OLED, and RTC. This research has proven that the accuracy of this device is feasible for SpO2 and BPM displayed on OLED. The device can be expanded by adding a sim card so that messages can be sent without connecting to android.

Based on the identification of the condition above, the author desire to design a Vital Sign Monitoring device for BPM and SpO2 Parameters with Notifications through the IoT-Based Telegram application. This device is used as a monitoring device that can be used anywhere and anytime, and so that patients or users can monitor their vital conditions which are displayed on the display, web thinger.io, forwarded to telegram if the patient's condition is not normal, and the indicator lights will light up differently. for each condition. Patients in the adult age range can use this device to relate well to medical personnel and receive timely care.

II. Materials and Methods

A. Experimental Setup

This study uses six normal subjects in relaxed conditions, and was randomly sampled also the data collection is repeated 6 times.

1) Materials and Tools

The study uses the MAX30100 (Gy-Max30100, Hongkong) as a digital sensor to detect oxygen saturation and heart rate. The MAX30100 is an integrated heart rate monitor and pulse oximetry sensor solution. It combines two LEDs, a photodetector, optimized optics, and low-noise analog signal

processing to detect pulse oximetry and heart rate signals [18]. The prepared sensor is placed on the patient's finger. Furthermore, two microcontrollers are used to process the device so that it can achieve the desired target. The Arduino Mega [19] microcontroller is for reading sensor data and communicating with IoT using the ESP32 Microcontroller [20]. LCD Character 20x4 is used to display values and an RGB LED that will light up according to the displayed data values. A Patient Monitor (Mindray, Beneheart D6, China) will be used to compare device values. The study is used a MAX30100 (Gy-Max30100, Hongkong). The MAX30100 is an integrated pulse oximetry and heart rate monitor sensor solution. It combines two LEDs, a photodetector, optimized optics, and low-noise analog signal processing to detect pulse oximetry and heart-rate signals [18]. The sensor was attached to the finger of the patient. Used two microcontrollers to process the device. The Arduino Mega Microcontroller [19] is to read the sensor data and communicate to the IoT using ESP32[20] Microcontroller. A 20x4 LCD Character to display the value and RGB LED that will light up according to the displayed data value. A Patient Monitor (Mindray, Beneheart D6, China) was used to compare the value from the device.

2) Experiment

In this study, after the design is complete, a trial will be carried out to obtain numerical results whose values will be compared with the IOT and LCD displays. The results obtained will then be compared using a calibrated vital sign monitor which was also installed during the trial on the same patient to test the device. Measurement of examination taking was carried out 6 (six) times in a row on 6 (six) different patients.

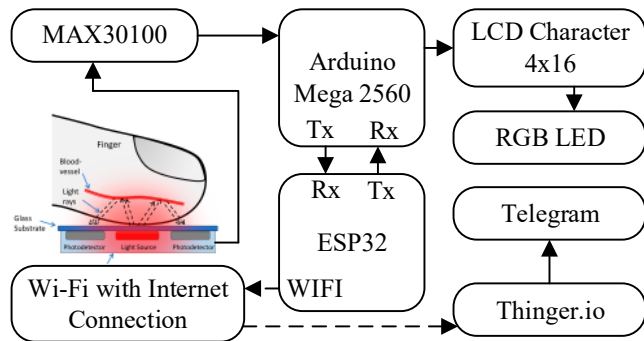


FIGURE 1 Diagram Blok

B. The Diagram Blok

In this research, the MAX30100 sensor will read the heart rate and oxygen saturation values attached to the finger. The results of the sensor readings will be processed in the Arduino Mega 2560 microcontroller as a data processor which will then be sent via serial communication to the ESP32 (FIGURE 1). Furthermore, wi-fi on the ESP32 will send data to the thinger.io server whose data can be accessed by health workers. If the data output from the parameter is not normal, a notification of the patient's vital status will be sent via telegram received by the health worker. In addition, the

RGB LED device will light up according to the patient's condition with the following information: red color means below normal, green color means normal, and blue color means above normal:

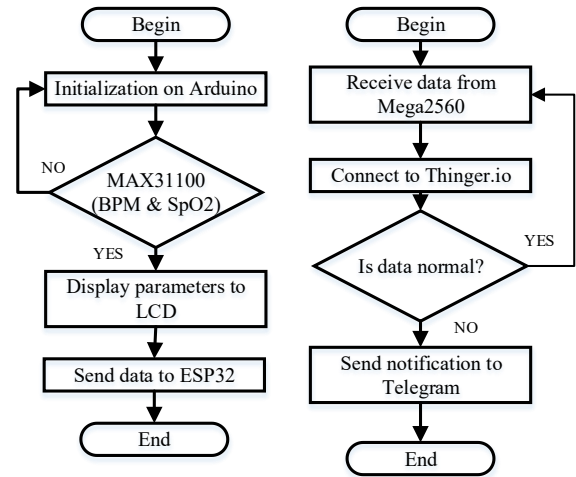


FIGURE 2 Flowchart of the Arduino Program

C. The flowchart

The Arduino program is built based on the flowchart as shown in FIGURE 2. When the on button is pressed, the initialization process occurs. The MAX30100 sensor will work to detect and calculate the value of heart rate (BPM) and oxygen saturation (SpO2) and the microcontroller Arduino Mega 2560 will process the data and send it to ESP32 while the data is displayed on the LCD Display. ESP32 will wait for the wifi to be connected. When the wifi is on, the data will be sent to Thingier.io, and there will be sent information to the telegram if the patient is in abnormal circumstances. The serial communication between Arduino Mega 2560 and ESP32 is shown in FIGURE 3 below.

III. Result

In this study, the device has been tested by comparing it to a patient monitor (Mindray, Beneheart D6, China) and MAX30100 (Gy-MAX30100,Hongkong) placed on the human body. The result shows that the device is feasible to be used by patients. FIGURE 4 is the monitoring vital sign design with the LCD Display and RGB LED.



FIGURE 4. The Monitoring Vital Sign Design

1) Measurement Reading Results

The measurement of the BPM value is shown in the display LCD, and thinger.io, and then they are

compared to the patient monitor. The measurement and the error are in TABLE 1.

TABLE 1

The BPM Measurement the Design and Standard Unit (Patient Monitor)

Respondent	\bar{X} Standard Unit (BPM)	\bar{X} Design (BPM)	Error(%)
1	74,5	74,16	0,004
2	104,67	104,83	0,0015
3	107	107,3	0,002
4	84	82,67	0,015
5	78,3	77,3	0,012
6	69,67	69,5	0,002

TABLE 2

The BPM Measurement the Design and Standard Unit (Patient Monitor)

Respondent	\bar{X} Standard Unit (%)	\bar{X} Design (%)	Error(%)
1	95,3	94,8	0,005
2	96,67	95,67	0,001
3	100	99,5	0,005
4	96,67	95,3	0,014
5	97,5	97,5	0
6	97,16	98,16	0,01

The measurement of SpO₂ value was also compared in this study, between the design and patient monitor. The result was shown in TABLE 2.

2) Thinger.io and Telegram

In FIGURE 5 above is a display of thinger.io compared to the design and also with the standard unit (patient monitor). Measurements were made on respondent 1 in a relaxed state. The display on Thinger.io and the serial monitor also appears on the display module with the same value, namely 72 bpm for heart rate, and 95% for respondent oxygen saturation.

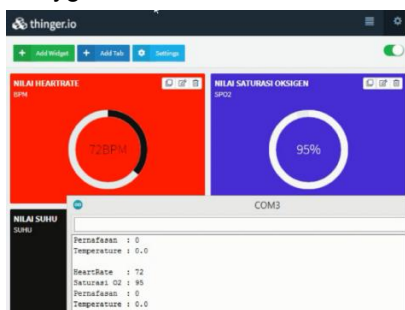


FIGURE 5 The thinger.io display



FIGURE 6. Telegram Notifications

in FIGURE 6 above, this is the chat display on the telegram if there is an abnormality in the patient's heart rate and oxygen saturation. Telegram programming is on ESP32 by giving calls to endpoints that have been provided by thinger.io as a facility. Given a millis function or pause for each telegram delivery.

IV. Discussion

In this study, a comparison of data was carried out to determine the Mean value and Error value of the device that was made. From the data that has been taken and the tests that have been carried out, the results of this study include BPM and SPO2 measurement data.

After accumulation, the average error in the SpO₂ parameter is = 0.01%, in the ECRI provisions regarding the maximum allowable error in the blood oxygen saturation (SpO₂) parameter, which is 1%, and the average error in the BPM parameter is = 0.015%, in the ECRI provisions regarding the maximum allowable error in the BPM parameter, which is 5% [21]. The results of the comparison of the module with the comparison device have an average error value that does not exceed the permissible limit according to their respective parameters. The resulting SpO₂ and BPM parameter values are displayed on the LCD, web thinger.io, telegram notifications equipped with light indicators on the device.

V. Conclusion

The purpose of this research is to design a Vital Sign Monitoring device for BPM and SpO₂ Parameters with Notifications through the IoT-Based Telegram application. The device has succeeded in detecting heart rate and oxygen saturation values satisfactorily and with sufficient accuracy. Furthermore, IoT thinger.io has succeeded in monitoring patient conditions and can be accessed by users and medical personnel in real-time in various places using the Telegram application. The resulting data has an error that does not exceed the allowable limit according to each parameter. The difference between the heart rate readings and oxygen saturation values on the device and patient monitor is 0.015% for heart rate and 0.01% for oxygen saturation. There is still a need to improve the ease of operation and also the use of competitive components so that they can be affordable for people.

References

- [1] E. L. Tysinger, "How Vital Are Vital Signs ? A Systematic Review of Vital Sign Compliance and Accuracy in Nursing," 2015.
- [2] Tortora, Gerard J., and Bryan H. Derrickson. *Principles of anatomy and physiology*. John Wiley & Sons, 2018.
- [3] Martínez-Nicolas, Antonio, Martin Meyer, Stefan Hunkler, Juan Antonio Madrid, Maria Angeles Rol, Andrea H. Meyer, Andy Schötzu, Selim Orgül, and Kurt Kräuchi. "Daytime variation in ambient temperature affects skin temperatures and blood pressure: ambulatory winter/summer comparison in healthy young women." *Physiology & behavior* 149 (2015): 203-211..
- [4] Fajkus, Marcel, Jan Nedoma, Radek Martinek, Vladimír Vasinek, Homer Nazeran, and Petr Siska. "A non-invasive multichannel hybrid fiber-optic sensor system for vital sign monitoring." *Sensors* 17, no. 1 (2017): 111..
- [5] Adiputra, R. R., S. Hadiyoso, and Y. Sun Hariyani. "Internet of things: Low cost and wearable SpO2 device for health monitoring." *International Journal of Electrical and Computer Engineering* 8, no. 2 (2018): 939.
- [6] Sahrul, Moch Sahrul Triandi Putra, and Torib Hamzah. "Patient Monitor for SpO2 and Temperature Parameters." *Journal of Electronics, Electromedical Engineering, and Medical Informatics* 1, no. 2 (2019): 7-12.
- [7] Narvaez, Jipcy Maurris N., and Glenn O. Avendaño. "Design and Implementation of Vital Signs Simulator for Patient Monitor." *Journal of Telecommunication, Electronic and Computer Engineering (JTEC)* 9, no. 2-4 (2017): 7-9.
- [8] F. Aktas, C. Ceken, and Y. E. Erdemli, "IoT-Based Healthcare Framework for Biomedical Applications," *J. Med. Biol. Eng.*, vol. 38, no. 6, pp. 966–979, 2018, doi: 10.1007/s40846-017-0349-7.
- [9] A. Wongjan, A. Julsereewong, and P. Julsereewong, "Continuous measurements of ECG and SpO2 for cardiology information system," in *Proceedings of the International MultiConference of Engineers and Computer Scientists*, 2009, vol. 2.
- [10] Nemcova, Andrea, Ivana Jordanova, Martin Varecka, Radovan Smisek, Lucie Marsanova, Lukas Smital, and Martin Vitek. "Monitoring of heart rate, blood oxygen saturation, and blood pressure using a smartphone." *Biomedical Signal Processing and Control* 59 (2020): 101928.
- [11] Mayya, Subramanya, Vivek Jilla, Vijay Narayan Tiwari, Mithun Manj Nath Nayak, and Rangavittal Narayanan. "Continuous monitoring of stress on smartphone using heart rate variability." In *2015 IEEE 15th international conference on bioinformatics and bioengineering (BIBE)*, pp. 1-5. IEEE, 2015.
- [12] De Ridder, Benjamin, Bart Van Rompaey, Jarl K. Kampen, Steven Haine, and Tinne Dilles. "Smartphone apps using photoplethysmography for heart rate monitoring: meta-analysis." *JMIR cardio* 2, no. 1 (2018): e8802..
- [13] Ho, Chi-Lin, Yun-Ching Fu, Ming-Chih Lin, Sheng-Ching Chan, Betau Hwang, and Sheng-Ling Jan. "Smartphone applications (apps) for heart rate measurement in children: comparison with electrocardiography monitor." *Pediatric cardiology* 35, no. 4 (2014): 726-731.
- [14] Turner, Justin, Chase Zellner, Tareq Khan, and Kumar Yelamarthi. "Continuous heart rate monitoring using smartphone." In *2017 IEEE International Conference on Electro Information Technology (EIT)*, pp. 324-326. IEEE, 2017.
- [15] Lagido, Ricardo Belchior, Joana Lobo, S. Leite, C. Sousa, Liliana Ferreira, and J. Silva-Cardoso. "Using the smartphone camera to monitor heart rate and rhythm in heart failure patients." In *IEEE-EMBS International Conference on Biomedical and Health Informatics (BHI)*, pp. 556-559. IEEE, 2014.
- [16] Lagido, Ricardo Belchior, Joana Lobo, S. Leite, C. Sousa, Liliana Ferreira, and J. Silva-Cardoso. "Using the smartphone camera to monitor heart rate and rhythm in heart failure patients." In *IEEE-EMBS International Conference on Biomedical and Health Informatics (BHI)*, pp. 556-559. IEEE, 2014..
- [17] E Lomaliza, Jean-Pierre, and Hanhoon Park. "A highly efficient and reliable heart rate monitoring system using smartphone cameras." *Multimedia Tools and Applications* 76, no. 20 (2017): 21051-21071.
- [18] Maxim Integrated, "Pulse Oximeter and Heart-Rate Sensor IC for Wearable Health," *Lect. Notes Energy*, vol. 38, pp. 1–29, 2014, [Online]. Available: www.maximintegrated.com.
- [19] Atmel, "Arduino Mega 2560 Datasheet," *Power*, pp. 1–7, 2015, [Online]. Available: <http://www.robotshop.com/content/PDF/ArduinoMega2560Datasheet.pdf>.
- [20] Espressif Systems, "ESP32 Series Datasheet." Shanghai Zhangjiang High-Tech Park, Shanghai, p. 53, 2018.
- [21] Perrotta, Andrew S., Andrew T. Jeklin, Ben A. Hives, Leah E. Meanwell, and Darren ER Warburton. "Validity of the elite HRV smartphone application for examining heart rate variability in a field-based setting." *The Journal of Strength & Conditioning Research* 31, no. 8 (2017): 2296-2302.

APPENDIX

1) The Listing Program For Arduino Mega 2560

In this paper, the software was divided into two programs which are for Arduino Mega and ESP32. The listing program for Arduino was shown in **Pseudocode: 1**. Which consisted of the program to read the data and send it to ESP32, and also to display the LCD and RGB LED.

Pseudocode: 1. Program to read the BPM and SpO2 and send the data to ESP32

```

1. #include <Wire.h>
2. #include "MAX30100_PulseOximeter.h"
3. #define REPORTING_PERIOD_MS 1000
4. uint32_t tsLastReport = 0;
5. int BPM, SPO;
6. PulseOximeter pox;
7.
8. SETUP:
9. Serial.begin(9600);
10. LOOP:
11. pox.update();
12. String minta = "";
13. while (Serial.available() > 0){
14.   minta += char(Serial.read());
15.   if (minta == "Y"){
16.     kirimdata();
17.     minta = "";
18.   }
19. KirimData:
20.   BPM = pox.getHeartRate();
21.   SPO = pox.getSpO2();
22.   String datakirim = String(BPM) + "#" + String(SPO);
   Serial.println(datakirim);

```

2) The Listing Program For Esp32

After the arduino mega gets and processes the sensor results, the ESP32 will receive the value which will be sent to Thingier.io which program will be shown in **Pseudocode: 2** below.

Pseudocode: 2. Program to receive the data and send it to Thingier.io and telegram.

```

1. #include <SoftwareSerial.h>
2. #include <ThingierESP32.h>
3. #include <Wire.h>

```

```

4. #define USERNAME "timothy0314"
5. #define DEVICE_ID "PROGRESS1"
6. #define          DEVICE_CREDENTIAL
7. "I8BGITB8bX$uY$"
8. ThingESP32          thing(USERNAME,
9. DEVICE_ID, DEVICE_CREDENTIAL);
10. const char * const ssid = "Indihome";
11. const char* const password = "maradika";
12. SoftwareSerial DataSerial(16,17);
13. unsigned long previousMillis = 0;
14. const long interval = 1500;
15. unsigned long millis3; //bpm
16. unsigned long millis4; //
17. unsigned long millis5; // spo
18. unsigned long millis6; //
19. String arrData[2];
20. int BPM,SPO;
21. SETUP:
22. Serial.begin(9600);
    DataSerial.begin(9600);
    thing.add_wifi(ssid,password);
        thing["BPM"] >> [](pson& out){
            out["BPM"] = BPM ;};
        thing["SPO2"] >> [](pson& out){
            out["SPO2"] = SPO ;};
    int indexnya =0;
LOOP:
    unsigned long currentMillis = millis();
    if(currentMillis - previousMillis >= interval){
        previousMillis = currentMillis;
        String data = "";
        while(DataSerial.available(>0){
            data += char(DataSerial.read());}
        char buf[sizeof(data)];
        data.trim();
        data.toCharArray(buf,sizeof(buf));
        char *p=buf;
        char *str;
        while((str=strtok_r(p,"#",&p))!=NULL){
            arrData[indexnya]=str;
            indexnya++;}
        if(indexnya>0){
            BPM          = arrData[0].toInt();
            SPO          = arrData[1].toInt();
            thing.stream(thing["BPM"]);
            thing.stream(thing["SPO"]);
            if (BPM != 0) {
                if (BPM < 60) {
                    millis3 = millis();
                    if (millis3 - millis4 > 30000) {
                        thing.call_endpoint("BPM");
                        millis4 = millis();}
                    if (BPM > 100) {
                        millis3 = millis();
                        if (millis3 - millis4 > 30000) {
                            thing.call_endpoint("BPM");
                            millis4 = millis();}}}}
            if (SPO != 0) {
                if (SPO < 95) {

```

```

millis5 = millis();
if (millis5 - millis6 > 30000) {
    thing.call_endpoint("SPO");
    millis6 = millis();}}}

```